

N5531X X-Series Measuring Receiver



N5531X
(Primary configuration)

N5531X
(Alternative configuration)

Conditions and Requirements

The Keysight N5531X X-Series measuring receiver offers 2 types of configurations: (1) Primary configuration- A “one-box” solution which is comprised of an N9030B PXA signal analyzer, multi-touch, with the N9091EMOE measuring receiver application, and a U5532C USB sensor module; and (2) Alternative configuration- A combination of an N9030B PXA with the N9091EMOE app, an N191xA EPM or P-Series power meter, and an N5532B sensor module. To achieve the optimal measurement results as specified, the best metrology practice must be applied and the required instrument conditions must be met.

PXA is the core instrument of the N5531X measuring receiver. The PXA instrument conditions stated in the PXA specification guide must be satisfied to meet the N5531X specifications.

Additional conditions required to meet specifications

- The system components are within their calibration cycle
- Tuned RF Level measurement is set to **High Accuracy Mode**; The measurements need to be complete within a time period of 20 minutes after setting the Reference Level
- Fast Mode is set to **Off** when performing modulation measurements
- For center frequency < 20 MHz, DC coupling is applied
- At least 2 hours of storage or operation at the operating temperature of 20 to 30 °C
- The PXA has been turned on at least 30 minutes with Auto Align On selected or if Auto Align Off is selected, Align All Now must be run:
 - Within the last 24 hours, and
 - Any time the ambient temperature changes more than 3 °C
 - After the analyzer has been at operating temperature at least 2 hours
- For analog modulation measurements, a direct connection between the PXA and the device under test (DUT) is required to achieve the best performance and meet the specifications for all test frequencies
- The following table summarizes PXA option and X-Series application selections under N5531X measuring receiver

Key features:

- Metrology-grade measurement accuracy
- Off-the-shelf, general-purpose instruments with specialized X-Series applications
- Best for signal source and step attenuator calibrations
- Abundant features with intuitive, easy-to-use multi-touch user interfaces
- Sensor modules covering up to 50 GHz with single input connection

Key measurements include:

- Frequency counter
- Absolute RF power
- Tuned RF level
- TRFL with tracking
- AM depth
- FM deviation
- PM deviation
- Modulation rate
- Modulation distortion
- Modulation SINAD
- Audio frequency
- Audio AC level
- Audio distortion
- Audio SINAD
- Auto carrier triggering
- CCITT filters

Category	Option Number	Description	Note
REQUIRED	N9030B-5xx	Any frequency options (e.g., 550)	
	N9030B-MPB	Microwave preselector bypass	Required for all frequency options except for 503
	N9030B-Pxx	Preamplifier, 100 kHz to the max frequency of PXA	
	N9030B-107	Audio input and digitizer	Required for audio analysis
	N9091EMOE	Measuring receiver application software	
OPTIONAL	N9030B-xxx	PXA options (e.g., N9030B-YAV)	Refer to N5531X configuration guide (5992-2675EN) and N9030B configuration guide (5992-1318EN) for more details
	N90xxEMOE	Most of X-Series applications (e.g., N9068EMOE)	
DISALLOWED	N9030B-RTS	Real-Time Wideband I/Q Data Streaming	Yet to be qualified in the production line
	N9030B-BBA	I/Q Baseband Inputs, Analog	Not compatible with Option N9030B-107 (Audio input and digitizer)

Key Specifications

1.0 Carrier frequency and bandwidth

Description	Specification	Supplemental Information
Carrier frequency		
Maximum frequency		
Option 503	3.6 GHz	RF/μW frequency option
Option 508	8.4 GHz	RF/μW frequency option
Option 513	13.6 GHz	RF/μW frequency option
Option 526	26.5 GHz	RF/μW frequency option
Option 544	44 GHz	mmW frequency option
Option 550	50 GHz	mmW frequency option
Minimum frequency		
AC coupled ¹	10 MHz	In practice, limited by the need to keep modulation sidebands from folding, and by the interference from LO feedthrough. For absolute RF power and TRFL measurements, the minimum frequency is limited by the power sensor module.
DC coupled	2 Hz	
Maximum information bandwidth (info BW)²		
Standard	25 MHz	
Option B40	40 MHz	
Option B85	85 MHz	
Option B1X	160 MHz	
Option B2X	255 MHz ³	
Option B5X	510 MHz ³	Not compatible with Option 107 (Audio input and digitizer)

1. AC Coupled is only applicable to frequency Options 503, 508, 513, and 526.
2. The maximum Info BW indicates the maximum operational BW, which depends on the analysis BW option equipped with the analyzer. However, the demodulation specifications only apply to the "IF BW" indicated in the FM, AM, and PM sections.
3. Under "Measuring Receiver" Mode, limited to 160 MHz maximum.

Key Specifications (continued)

1.1 Frequency modulation (FM)

Conditions required to meet specifications:

- Peak FM Deviation ≥ 200 Hz
- $\beta \geq 0.2$ or FM Deviation ≥ 200 Hz whichever is greater, and $\beta \leq 20000$ or FM Deviation ≤ 1 MHz whichever is smaller where, β is modulation index and defined as (FM Deviation)/(FM Rate)
- Info Bandwidth (IF BW): ≤ 8 MHz for center frequency (f_c) between 100 kHz and 3.6 GHz,
 ≤ 3.5 MHz for $f_c > 3.6$ GHz
- SINAD BW: (IF BW)/2
- Single tone: sinusoid modulation

Description	Specification	Supplemental Information
Input power range	-24 to +30 dBm	
FM rate range ¹	100 kHz $\leq f_c < 3.6$ GHz 3.6 GHz $\leq f_c < 50$ GHz	10 Hz to 400 kHz 10 Hz to 200 kHz
Peak FM deviations range ¹	100 kHz $\leq f_c \leq 50$ GHz	1 MHz maximum
FM deviation accuracy²		
Frequency range	β	
100 kHz to 3.6 GHz	$\geq 0.2, \leq 100$ > 100	$\pm (0.35\% \text{ of reading} + 0.2\% \times \text{rate})$ $\pm 0.8\% \text{ of reading}$
3.6 to 8.4 GHz	$\geq 0.2, \leq 100$ > 100	$\pm (0.7\% \text{ of reading} + 0.2\% \times \text{rate})$ $\pm 2\% \text{ of reading}$
8.4 to 17.1 GHz	$\geq 0.2, \leq 100$ > 100	$\pm (0.7\% \text{ of reading} + 0.3\% \times \text{rate})$ $\pm 2.5\% \text{ of reading}$
17.1 to 34.5 GHz	$\geq 0.2, \leq 100$ > 100	$\pm (0.8\% \text{ of reading} + 0.3\% \times \text{rate})$ $\pm 3.0\% \text{ of reading}$
34.5 to 50 GHz	$\geq 0.2, \leq 100$ > 100	$\pm (1.4\% \text{ of reading} + 0.5\% \times \text{rate})$ $\pm 4.0\% \text{ of reading}$
AM rejection (AM signal (Rate = 1kHz, Depth = 50%), 50 Hz to 3 kHz BW)		
Frequency range	Max peak deviation	
100 kHz to 3.6 GHz	2.8 Hz	
3.6 to 13.6 GHz	9.6 Hz	
13.6 to 17.1 GHz	9.9 Hz	
17.1 to 26.5 GHz	10.8 Hz	
26.5 to 34.5 GHz	11.5 Hz	
34.5 to 50 GHz	13.5 Hz	
Residual FM³ (50 Hz to 3 kHz BW)		
RF frequency		
100 kHz to 3.6 GHz	< 1.2 Hz (rms)	
3.6 to 8.4 GHz	< 3.9 Hz (rms)	
8.4 to 13.6 GHz	< 4.2 Hz (rms)	
13.6 to 17.1 GHz	< 4.4 Hz (rms)	
17.1 to 26.5 GHz	< 4.9 Hz (rms)	
26.5 to 34.5 GHz	< 5.7 Hz (rms)	
34.5 to 50 GHz	< 6.7 Hz (rms)	
Detectors	Available: +peak, -peak, \pm peak/2, peak hold, rms	

1. The modulation rates and the peak deviations that the system is capable of measuring are governed by the instrument's IFBW (Information Bandwidth) setting. Their relationship is described by the equation: Peak deviation (in Hz) = IFBW/2 - modulation rate.
2. When the carrier frequency f_c is less than 10 MHz, to avoid the 0 Hz frequency wrap-around, the f_c and IFBW must be chosen to satisfy $[f_c - (\text{IFBW}/2)] > 100$ kHz.
3. The Residual FM specification is a warranted traceable worst-case figure for the entire band. For most instruments, at most frequencies, the actual residual FM performance is usually much better (lower). When testing the Residual FM of a DUT, the reading indicated by N9091EM0E is the combined noise of the DUT and the MMR-X analyzer. If the FM noise of the DUT and MMR-X are uncorrelated (normally the case), then these two contributors can only add to each other in a RSS (Root-Sum-Squared) manner. Therefore, we can say with high confidence that the FM noise of the DUT is no greater than the Residual FM indicated by N9091EM0E.

Key Specifications (continued)

1.2 Amplitude modulation

Conditions required to meet specifications

- Info BW (IF BW) \leq 1MHz
- IF BW: 15 times of AM rate (when AM rate \leq 50 kHz) or 10 times of AM rate (when 50 kHz $<$ AM rate \leq 100 kHz)
- SINAD BW: (IF BW)/2
- Single tone: sinusoid modulation

Description	Specification	Supplemental Information
Input power range	-24 to +30 dBm	
AM rate range ¹	$100 \text{ kHz} \leq f_c < 50 \text{ GHz}$	10 Hz to 100 kHz
AM depth range	1 to 99%	Capable of measuring AM depth range of 0 to 100%.
AM depth accuracy²		
Frequency range	Depths	
100 kHz to 3.6 GHz	1% to 99%	\pm (0.1% of reading + 0.07%)
3.6 to 13.6 GHz	5% to 99%	\pm (0.1% of reading + 0.10%)
13.6 to 17.1 GHz	5% to 99%	\pm (0.1% of reading + 0.12%)
17.1 to 26.5 GHz	5% to 99%	\pm (0.15% of reading + 0.12%)
26.5 to 34.5 GHz	5% to 99%	\pm (0.15% of reading + 0.16%)
34.5 to 50 GHz	5% to 99%	\pm (0.15% of reading + 0.35%)
Flatness (AM depth \geq 10%)		
Frequency range		
100 kHz to 3.6 GHz	\pm 0.25% of reading	
3.6 to 8.4 GHz	\pm 0.60% of reading	
8.4 to 17.1 GHz	\pm 0.65% of reading	
17.1 to 26.5 GHz	\pm 0.80% of reading	
26.5 to 34.5 GHz	\pm 0.90% of reading	
34.5 to 50 GHz	\pm 0.90% of reading	10 Hz \leq AM rate \leq 10 kHz
FM rejection (FM signal (Rate = 1 kHz, Deviation = 50 KHz), 50 Hz to 3 kHz BW)³		
Frequency range		
100 kHz to 34.5 GHz	0.04%	
34.5 to 50 GHz	0.08%	
Residual AM⁴ (300 Hz to 3 kHz BW)		
100 kHz to 3.6 GHz	0.01% (rms)	
3.6 to 34.5 GHz	0.04% (rms)	
34.5 to 50 GHz	0.05% (rms)	
Detectors	Available: +peak, -peak, \pm peak/2, peak hold, rms	

1. When the carrier frequency f_c is less than 10 MHz, to avoid the 0 Hz frequency wrap-around, the f_c and IF BW must be chosen to satisfy $\text{IF BW} < 2 \times (f_c - 100 \text{ kHz})$. For peak measurement only: AM accuracy may be affected by distortion generated by the measuring receiver. In the worst case this distortion can decrease accuracy by 0.1% of reading for each 0.1% of distortion.
2. Flatness is the relative variation in indicated AM depth versus rate for a constant carrier frequency and depth.
3. FM rejection (also known as "incidental AM" due to FM/PM) describes the instrument's AM reading for an input that is strongly FMed (with no AM); this specification includes contributions from residual AM. FM signal (Rate = 1 kHz, Deviation = 50 kHz), HPF = 300 Hz, LPF = 3 kHz, Channel BW = 420 kHz. Conditions that would constrain AM depth, or constrain the rate of modulation, do not apply to incidental AM.
4. Follow this procedure to verify this specification: Input a clean CW signal (0 dBm) to the measuring receiver; Manually tune the frequency to the input signal; Set the PXA parameters as follows, (1) IF BW = 6 kHz, (2) Detector type = RMS, (3) High Pass Filter = 50 Hz, (4) Low Pass Filter = 3 kHz, (5) Set **RF Input Ranging to Man**, and decrease the input attenuation at 2 dB/step until **SigHi** message appears, and then back off 2 dB for the **SigHi** message to disappear.

Key Specifications (continued)

1.3 Phase modulation (PM)

Conditions required to meet specifications:

- Info BW (IF BW) \leq 3.5 MHz
- HPF = 50 Hz always On (unless otherwise stated)
- SINAD BW: (IF BW)/2
- Single tone: sinusoid modulation
- Center frequency (f_c): \geq 100 kHz

Description	Specification	Supplemental Information
Input power range	-24 to +30 dBm	
PM rate range ¹	100 kHz \leq f_c < 50 GHz	200 Hz to 100 kHz
Peak phase deviation ^{2,3}	100 kHz \leq f_c < 50 GHz	0.2 to 25,000 radians
PM accuracy		
Frequency range		
100 kHz to 3.6 GHz		\pm (0.1% x reading + 2 mrad)
3.6 to 13.6 GHz		\pm (0.1% x reading + 3 mrad)
13.6 to 17.1 GHz		\pm (0.1% x reading + 4 mrad)
17.1 to 26.5 GHz		\pm (0.1% x reading + 6 mrad)
26.5 to 34.5 GHz		\pm (0.1% x reading + 9 mrad)
34.5 to 50 GHz		\pm (0.1% x reading + 10 mrad)
AM rejection (AM signal (Rate = 1kHz, Depth = 50%), 50 Hz to 3 kHz BW)		
Frequency range		
100 kHz to 3.6 GHz		0.0030 rad
3.6 to 8.4 GHz		0.0054 rad
8.4 to 13.6 GHz		0.0081 rad
13.6 to 17.1 GHz		0.0105 rad
17.1 to 26.5 GHz		0.0159 rad
26.5 to 34.4 GHz		0.0199 rad
34.4 to 50 GHz		0.0286 rad
Residual PM⁴ (50 Hz to 3 kHz BW)		
Frequency range		
100 kHz to 3.6 GHz		< 0.0017 rad (rms)
3.6 to 8.4 GHz		< 0.0032 rad (rms)
8.4 to 13.6 GHz		< 0.0048 rad (rms)
13.6 to 17.1 GHz		< 0.0060 rad (rms)
17.1 to 26.5 GHz		< 0.0091 rad (rms)
26.5 to 34.4 GHz		< 0.0117 rad (rms)
34.4 to 50 GHz		< 0.0165 rad (rms)
Detectors		Available: +peak, -peak, \pm peak/2, peak hold, rms

1. Below 500 Hz PM rate, set the HFP to "None" to meet the PM deviation accuracy specifications.
2. The f_c and IF BW must be chosen to satisfy $IF\ BW < 2x(f_c - 100\ kHz)$.
3. The maximum peak deviation that the instrument is capable of measuring depends on the IF BW setting and the modulation rate of the signal-under-test. The relationship is described by the equation: Max peak deviation (in radians) = $[IF\ BW / (2 \times \text{modulation rate in Hz})] - 1$.
4. The Residual PM specification is a warranted traceable worst-case figure for the entire band. For most instruments, at most frequencies, the actual residual PM performance is usually much better (lower). When testing the Residual PM of a DUT, the reading indicated by N9091EM0E is the combined noise of the DUT and the MMR-X analyzer. If the phase noise of the DUT and MMR-X are uncorrelated (normally the case), then these two contributors can only add to each other in a RSS (Root-Sum-Squared) manner. Therefore, we can say with high confidence that the phase noise of the DUT is no greater than the Residual PM indicated by N9091EM0E.

Key Specifications (continued)

1.4 RF frequency counter

Description	Specification	Supplemental Information
RF frequency range	Refer to Section 1.0	
Sensitivity ¹		In Auto mode
100 kHz ≤ f _c < 3.6 GHz	0.4 mV _{rms} (–55 dBm)	
3.6 GHz ≤ f _c ≤ 26.5 GHz	1.3 mV _{rms} (–45 dBm)	
26.5 GHz ≤ f _c ≤ 50 GHz	4.0 mV _{rms} (–35 dBm)	
Maximum resolution	0.001 Hz	
Accuracy ²	± (readout frequency x rfa + 0.100 Hz) ³	At defaulted measurement settings.
Accuracy (for f _c < 100 MHz) ⁴	± (readout freq. x rfa + 0.002 Hz) ³	± (readout freq. x rfa + 0.001 Hz) @ 99 percentile, or ≈2.576σ
Modes		Frequency and frequency error (manual tuning)
Sensitivity in manual tuning mode		Using manual ranging and changing RBW settings, sensitivity can be increased to approximately –100 dBm.

1.5 Audio input⁵

Description	Specification	Supplemental Information
Frequency range	20 Hz to 250 kHz	Starting from 5 Hz for “DC coupled”
Input impedance		100 kΩ (nominal)
Maximum safe input level		
AC coupled	7 V _{rms} or 20 VDC	
DC coupled	7 V _{rms} or 0 VDC	

1.6 Audio frequency counter⁵

Description	Specification	Supplemental Information
Frequency range		
AC coupled	20 Hz to 250 kHz	
DC coupled		5 Hz to 250 kHz (nominal)
Accuracy ⁶		
f < 1 kHz	± (0.02 Hz + f x rfa) ³	
f ≥ 1 kHz	± (3 counts of the first 6 significant digits + f x rfa) ³	
Resolution	0.01 Hz (8 digits)	
Sensitivity	≤ 5 mV	

1.7 Audio AC level (RMS)⁵

Description	Specification	Supplemental Information
Frequency range		
AC coupled	20 Hz to 250 kHz	
DC coupled		5 Hz to 250 kHz (nominal)
Measurement level range	100 mV _{rms} to 3 V _{rms}	
Accuracy	1% of reading	
Detector mode		RMS

- Instrument condition: RBW ≤ 1 kHz, “Auto” mode.
- Verified at 1 GHz with RBW = 1 kHz, gate time = 0.1 s (autocoupled), SNR = 50 dB. rfa = Internal reference frequency accuracy.
- rfa = Internal reference frequency accuracy. See the “Internal Time Base Reference” section in the PXA specification guide for the Internal Reference Frequency Accuracy (rfa).
- For the special case of f_c < 100 MHz, RBW = 300 Hz, and gate time = 0.5 s, the second term is < 0.002 Hz (3-sigma). The 0.002 Hz term includes noisiness as well as mean errors that occur at some frequencies, and thus cannot necessarily be reduced with averaging.
- All audio measurements require PXA Option 107. All audio specifications are for “AC Coupled” path and nominally apply to “DC Coupled” path (unless stated otherwise).
- Follow this procedure to verify this specification: Set an input audio signal at 100 mV. Set the PXA as follows: (1) Auto Level, (2) Auto IF BW, (3) LP is greater than the audio frequency, (4) HPF = 300 Hz or less than the audio frequency, and (5) Average = 5 Repeat.

1.8 Audio distortion¹

Description		Specification	Supplemental Information
Display range (20 Hz to 250 kHz)		0.01 to 100% (-80 to 0 dB)	Display range starts from 5 Hz for "DC coupled"
Accuracy ²	AC coupled	±1 dB of reading (20 Hz to 20 kHz) ±2 dB of reading (20 to 80 kHz ³)	± 0.3 dB of reading (nominal, 20 Hz to 200 kHz)
	DC coupled		±0.7 dB of reading (nominal, 5 Hz to 20 Hz) ±0.3 dB of reading (nominal, 20 Hz to 200 kHz)
Residual noise and distortion		< 0.3% (-50.4 dB)	<0.063% (-64 dB) (nominal)
Total noise			-73.2 dB characteristic performance
Total distortion			-74.8 dB characteristic performance

1.9 Audio SINAD¹

Description		Specification	Supplemental Information
Display range (20 Hz to 250 kHz)		0.00 to 80 dB	Display range starts from 5 Hz for "DC coupled"
Display resolution		0.001 dB	
Accuracy	AC coupled	±1 dB of reading (20 Hz to 20 kHz) ±2 dB of reading (20 to 80 kHz ³)	± 0.3 dB of reading (nominal, 20 Hz to 200 kHz)
	DC coupled		±0.7 dB of reading (nominal, 5 Hz to 20 Hz) ±0.3 dB of reading (nominal, 20 Hz to 200 kHz)
Residual noise and distortion		50.4 dB	64 dB (nominal)
Total noise			73.2 dB characteristic performance
Total distortion			74.8 dB characteristic performance

1.10 Audio filters¹

Description		Specification	Supplemental Information
Filter flatness			Cutoff frequency (nominal); filter type
50 Hz high-pass filter		< ± 1% at rates > 175 Hz	-3 dB @ 50 Hz HPF; 2-pole Butterworth
300 Hz high-pass filter		< ± 1% at rates > 950 Hz	-3 dB @ 300 Hz HPF; 2-pole Butterworth
400 Hz high-pass filter		< ± 1% at rates > 550 Hz	-3 dB @ 400 Hz HPF; 10-pole Butterworth
3 kHz low-pass filter		< ± 1% at rates < 1.5 kHz	-3 dB @ 3 kHz LPF; 5-pole Butterworth
15 kHz low-pass filter		< ± 1% at rates < 9 kHz	-3 dB @ 15 kHz LPF; 5-pole Butterworth
30 kHz low-pass filter		< ± 1% at rates < 13.5 kHz	-3 dB @ 30 kHz LPF; 3-pole Butterworth
80 kHz low-pass filter		< ± 1% at rates < 38.5 kHz	-3 dB @ 80 kHz LPF; 3-pole Butterworth
> 300 kHz low-pass filter		< ± 1% at rates < 285 kHz	-3 dB @ 300 kHz LPF; 3-pole Butterworth
CCITT weighting filter		CCITT recommendation P53	
Deviation from the ideal		± 0.2 dB at 800 Hz; ± 1.0 dB, 300 Hz to 3 kHz	
CCITT filter response		± 2.0 dB, 50 to 300 Hz and 3 to 3.5 kHz; ± 3.0 dB, 3.5 to 5 kHz	
De-emphasis filters		25 μs, 50 μs, 75 μs, and 750 μs	De-emphasis filters are single-pole, low-pass filters with nominal -3 dB frequencies of: 6,366 Hz for 25 μs, 3,183 Hz for 50 μs, 2,122 Hz for 75 μs, and 212 Hz for 750 μs.
Deviation from ideal de-emphasis filter		< 0.4 dB, or < 3°	Applicable to 25 μs, 50 μs, and 75 μs filters. With 3 kHz Low-Pass filter and IFBW Mode set to minimal.

- All audio measurements require PXA Option 107. All audio specifications are for "AC Coupled" path and nominally apply to "DC Coupled" path (unless stated otherwise).
- Verified in dB; can be converted into linear term in % using formula of % = $[1 - 10^{-(A \text{ dB} \div 20)}] \times 100\%$.
- Verified up to 80 kHz due to the limitation of test equipment.

1.11 RF power^{1,2}

The Keysight N5531X measuring receiver system with the U5532C USB sensor modules or the N5532B/A sensor modules performs RF power measurements from -10 dBm (100 μ W) to +30 dBm (1 W). When the N5532B/A sensor modules are used, the Keysight EPM Series power meters (N1913A, N1914A) or P-Series power meter (N1911A, N1912A), or legacy power meter (E4446A, E4447A, E4448B, E4449B) is required.

Description		Specification				Supplemental Information			
RF power accuracy (dB)									
Power meter range 1 (+20 to +30 dBm)					Typicals				
		Sensor module options				Sensor module options			
		504	518	526	550	504	518	526	550
	100 kHz $\leq f_c \leq$ 10 MHz	± 0.287	–	–	–	± 0.146	–	–	–
	10 MHz $< f_c \leq$ 30 MHz	± 0.287	± 0.287	$\pm 0.287^2$	–	± 0.146	± 0.146	$\pm 0.146^2$	–
	30 MHz $< f_c \leq$ 2 GHz	± 0.287	± 0.287	± 0.287	± 0.265	± 0.146	± 0.146	± 0.146	± 0.135
	2 GHz $< f_c \leq$ 4.2 GHz	± 0.302	± 0.287	± 0.302	± 0.279	± 0.154	± 0.154	± 0.154	± 0.142
	4.2 GHz $< f_c \leq$ 18 GHz	–	± 0.466	± 0.468	± 0.342	–	± 0.240	± 0.241	± 0.175
	18 GHz $< f_c \leq$ 26.5 GHz	–	–	± 0.386	± 0.332	–	–	± 0.198	± 0.170
	26.5 GHz $< f_c \leq$ 50 GHz	–	–	–	± 0.363	–	–	–	± 0.186
Power meter range 2 (0 to +20 dBm)					Typicals				
		Sensor module options				Sensor module options			
		504	518	526	550	504	518	526	550
	100 kHz $\leq f_c \leq$ 10 MHz	± 0.222	–	–	–	± 0.113	–	–	–
	10 MHz $< f_c \leq$ 30 MHz	± 0.222	± 0.222	$\pm 0.222^2$	–	± 0.113	± 0.113	$\pm 0.113^2$	–
	30 MHz $< f_c \leq$ 2 GHz	± 0.222	± 0.222	± 0.222	± 0.191	± 0.113	± 0.113	± 0.113	± 0.097
	2 GHz $< f_c \leq$ 4.2 GHz	± 0.242	± 0.242	± 0.242	± 0.211	± 0.123	± 0.123	± 0.123	± 0.107
	4.2 GHz $< f_c \leq$ 18 GHz	–	± 0.432	± 0.433	± 0.291	–	± 0.222	± 0.232	± 0.148
	18 GHz $< f_c \leq$ 26.5 GHz	–	–	± 0.342	± 0.279	–	–	± 0.175	± 0.142
	26.5 GHz $< f_c \leq$ 50 GHz	–	–	–	± 0.316	–	–	–	± 0.161
Power meter range 3 (-5 to 0 dBm)					Typicals				
		Sensor module options				Sensor module options			
		504	518	526	550	504	518	526	550
	100 kHz $\leq f_c \leq$ 10 MHz	± 0.220	–	–	–	± 0.112	–	–	–
	10 MHz $< f_c \leq$ 30 MHz	± 0.220	± 0.219	$\pm 0.220^2$	–	± 0.112	± 0.111	$\pm 0.112^2$	–
	30 MHz $< f_c \leq$ 2 GHz	± 0.220	± 0.219	± 0.220	± 0.189	± 0.112	± 0.111	± 0.112	± 0.096
	2 GHz $< f_c \leq$ 4.2 GHz	± 0.240	± 0.240	± 0.240	± 0.209	± 0.122	± 0.122	± 0.122	± 0.106
	4.2 GHz $< f_c \leq$ 18 GHz	–	± 0.430	± 0.432	± 0.289	–	± 0.221	± 0.222	± 0.148
	18 GHz $< f_c \leq$ 26.5 GHz	–	–	± 0.341	± 0.277	–	–	± 0.174	± 0.141
	26.5 GHz $< f_c \leq$ 50 GHz	–	–	–	± 0.315	–	–	–	± 0.161
Power meter range 4 (-10 to -5 dBm)					Typicals				
		Sensor module options				Sensor module options			
		504	518	526	550	504	518	526	550
	100 kHz $\leq f_c \leq$ 10 MHz	± 0.229	–	–	–	± 0.117	–	–	–
	10 MHz $< f_c \leq$ 30 MHz	± 0.229	± 0.229	$\pm 0.229^2$	–	± 0.117	± 0.117	$\pm 0.117^2$	–
	30 MHz $< f_c \leq$ 2 GHz	± 0.229	± 0.229	± 0.229	± 0.200	± 0.117	± 0.117	± 0.117	± 0.102
	2 GHz $< f_c \leq$ 4.2 GHz	± 0.249	± 0.249	± 0.249	± 0.219	± 0.127	± 0.127	± 0.127	± 0.111
	4.2 GHz $< f_c \leq$ 18 GHz	–	± 0.435	± 0.437	± 0.296	–	± 0.224	± 0.225	± 0.151
	18 GHz $< f_c \leq$ 26.5 GHz	–	–	± 0.347	± 0.285	–	–	± 0.178	± 0.145
	26.5 GHz $< f_c \leq$ 50 GHz	–	–	–	± 0.321	–	–	–	± 0.164
RF power resolution	Display resolution	0.001 dB							
Instrumentation accuracy	Logarithmic	± 0.02 dB							
	Linear	$\pm 0.5\%$							

- The N5531X RF Power Accuracy is derived from the power meter accuracy. The parameters listed in this section are components used to calculate the RF Power Accuracy. Fundamentals of RF and Microwave Power Measurements (5988-9215EN) does an excellent job of explaining how the components are combined to derive an overall accuracy number. The resulting calculation yields ± 0.190 to ± 0.297 dB when measuring a +10 dBm signal and ignoring DUT mismatch. Assuming 1.5:1 DUT SWR, the calculation would return a typical accuracy of ± 0.213 to ± 0.387 dB (depending on the frequency range and power under test). Absolute and relative accuracy specifications do not include mismatch uncertainty.
- For U5532C USB sensor modules only.

1.11 RF power (continued)

Description		Specification	Supplemental Information
Input SWR			
U5532C Option 504	100 kHz to 2 GHz	< 1.10:1 ($\rho = 0.048$)	
N5532B Option 504	2 GHz to 4.2 GHz	< 1.28:1 ($\rho = 0.123$)	
U5532C Option 518	10 MHz to 2 GHz	< 1.10:1 ($\rho = 0.048$)	
N5532B Option 518	2 GHz to 18 GHz	< 1.28:1 ($\rho = 0.123$)	
U5532C Option 526	10 MHz to 30 MHz	< 1.10:1 ($\rho = 0.048$)	For U5532C-526 only
N5532B Option 526	30 MHz to 2 GHz	< 1.10:1 ($\rho = 0.048$)	
	2 GHz to 18 GHz	< 1.28:1 ($\rho = 0.123$)	
	18 GHz to 26.5 GHz	< 1.40:1 ($\rho = 0.167$)	
U5532C Option 550	30 MHz to 2 GHz	< 1.10:1 ($\rho = 0.048$)	
N5532B Option 550	2 GHz to 18 GHz	< 1.28:1 ($\rho = 0.123$)	
	18 GHz to 26.5 GHz	< 1.40:1 ($\rho = 0.167$)	
	26.5 GHz to 33 GHz	< 1.55:1 ($\rho = 0.216$)	
	33 GHz to 40 GHz	< 1.70:1 ($\rho = 0.259$)	
	40 GHz to 50 GHz	< 1.75:1 ($\rho = 0.272$)	
Zero set and measurement noise ¹	N5532B	± 680 nW	
	U5532C	± 500 nW	
Zero drift of sensors (1 hour, at constant temperature after 24 hour warm-up)	N5532B	< 100 nW	
	U5532C	< 70 nW	
RF power ranges of N5531X with U5532C or N5532B sensor modules		-20 dBm (10 μ W) to +30 dBm (1 W)	One range for power sensors
Response time (0 to 99% of reading)			150 ms x number of averages (nominal)
Displayed units		Watts, dBm, or Volts	

1. Since zero set and measurement noise cannot be separated, these two components are combined as one error term.

Key Specifications (continued)

TRFL specification nomenclature

The tuned RF level measurement uncertainty is represented primarily by two regions. For high signal-to-noise (S/N) measurements, the uncertainty is dominated by the linearity of the measuring receiver. For low S/N measurements, the measurement uncertainty is dominated by the noise of the measuring receiver being added to the measured signal. The input power at which the uncertainty switches from linearity dominated to noise dominated is labeled as Residual noise threshold. The minimum power level is defined as the noise floor of the measuring receiver system.

Additionally, there are 2 range-to-range change uncertainties known as Range 2 Uncertainty and Range 3 Uncertainty, respectively. Range 2 Uncertainty occurs when the measuring receiver switches from Range 1 to Range 2, and Range 3 uncertainty from Range 2 to Range 3. They are additive uncertainties applied to all measurements whose input powers across Range Switch Level.

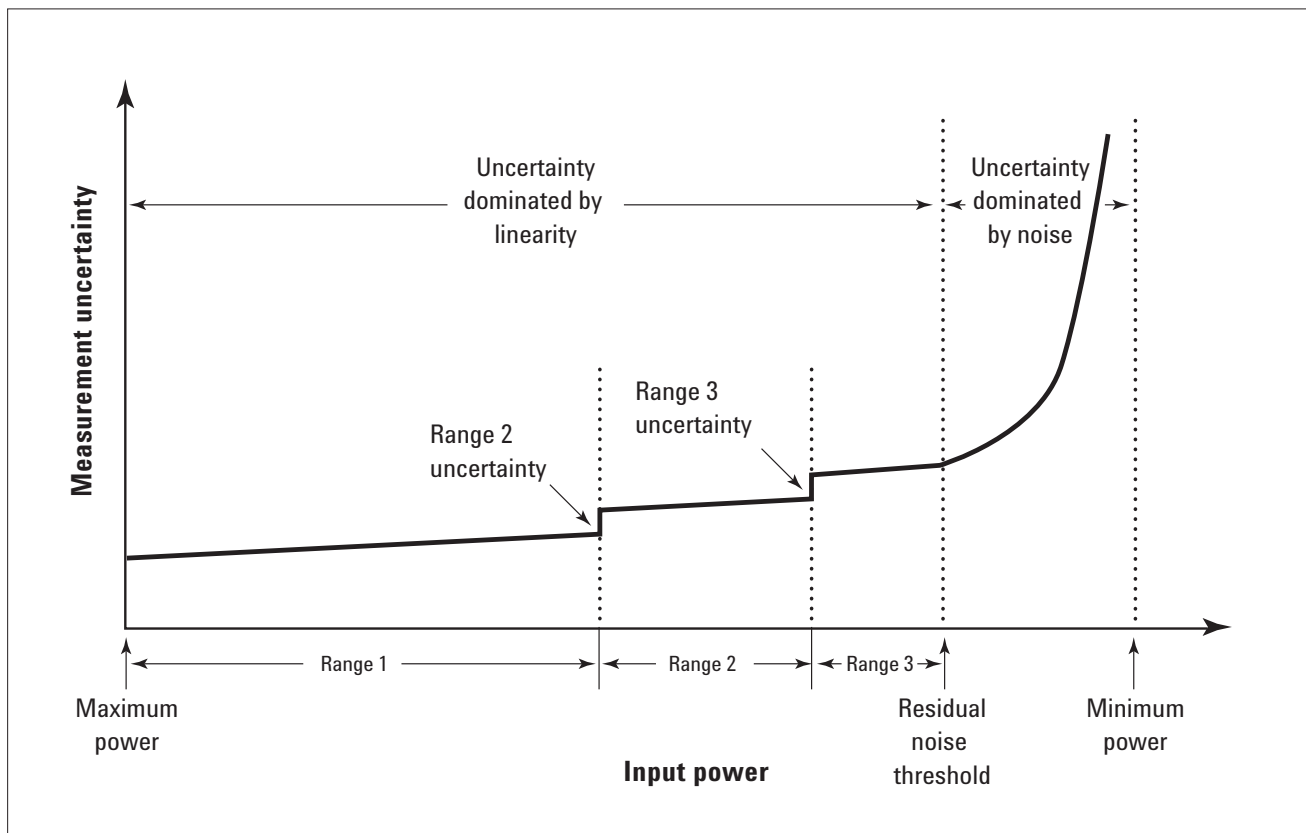


Figure 1. Measurement uncertainty vs. input power relationship

Key Specifications (continued)

1.12 Tuned RF level^{1, 2, 3}

Note: While the Tuned RF level specifications listed below are for IFBW settings of 75 Hz and 10 Hz, the IFBW in N5531X can also be set to 30 kHz or 200 kHz. The wider IFBW is capable of measuring sources with some degree of frequency instability by trading off measurement sensitivity.

For sources with frequency instability greater than 100 kHz, use the Tuned RF Level with Tracking measurement. When using the Tuned RF Level with Tracking, the following additional amplitude error must be applied due to FFT frequency response as the signal drifts within the tracking range: $\pm (0.15 \text{ dB} + 0.1 \text{ dB/MHz of span})$ to a max of $\pm 0.40 \text{ dB}$, where span is equivalent to the tracking range setting in the measurement. The Tuned RF Level with Tracking measurement upper frequency limit = 3.6 GHz. For the Tuned RF Level with Tracking, the minimum power = $10 * \log [\text{Integrated BW} / (75 \text{ Hz} * 1.06)]$, relative to the specified 75 Hz minimum power level.

Description	Specification	Supplemental Information	
Power range			
Maximum power	Preamp off	+30 dBm	
	Preamp on	+30 dBm	For Opt N9030B-503
		+24 dBm	For Opt 9030B-508/513/526
		+20 dBm	For Opt N9030B-544/550
Minimum power (dBm)⁴			
Opt N9030B-503/508/513/526	75 Hz IFBW⁵	10 Hz IFBW⁶	
Frequency range	Preamp On	Preamp On	
100 to 200 kHz	-123.0	-137.8	Band 0
200 to 500 kHz	-126.0	-140.8	Band 0
500 kHz to 1 MHz	-130.0	-144.8	Band 0
1 to 10 MHz	-132.0	-146.8	Band 0
10 MHz to 2.1 GHz	-136.0	-150.8	Band 0
2.1 to 3.6 GHz	-134.0	-148.8	Band 0
3.5 to 8.4 GHz	-130.2	-145.0	Band 1
8.3 to 13.6 GHz	-129.2	-144.0	Band 2
13.5 to 16.9 GHz	-123.2	-138.0	Band 3
16.9 to 20 GHz	-121.2	-136.0	Band 4
20 to 26.5 GHz	-106.7	-121.5	Band 4
Minimum power (dBm)⁴			
Opt N9030B-544/550	75 Hz IFBW⁵	10 Hz IFBW⁶	
Frequency range	Preamp On	Preamp On	
100 to 200 kHz	-123.0	-137.8	Band 0
200 to 500 kHz	-126.0	-140.8	Band 0
500 kHz to 1 MHz	-128.0	-142.8	Band 0
1 to 10 MHz	-132.0	-146.8	Band 0

1. PXA Option N9030B-MPB is required to perform Tuned RF Level measurements above 3.6 GHz.

2. These specifications are valid when the measuring receiver input is a CW tone and operating temperature is within the range of 20 to 30 °C.

3. Absolute and relative accuracy specifications do not include mismatch uncertainty.

4. With 30 kHz and 200 kHz IF bandwidth (IFBW), TRFL minimum power level will be degraded by a factor of $10 \log(\text{IFBW}/75 \text{ Hz})$, relative to the specified 75 Hz minimum power level. This will result in a degradation of 26 dB for the 30 kHz IFBW and 34 dB for the 200 kHz IFBW.

5. With 75 Hz IFBW setting selected, the measurement automatically switches the RBW to the 30 Hz setting for SNR values < 10 dB.

6. With 10 Hz IFBW setting selected, the measurement automatically switches the RBW to the 1 Hz setting for SNR values < 10 dB.

Key Specifications (continued)

1.12 Tuned RF level^{1, 2, 3} (continued)

Minimum power (dBm) ⁴			
Opt N9030B-544/550	75 Hz IFBW ⁵	10 Hz IFBW ⁶	
Frequency range	Preamp On	Preamp On	
10 MHz to 2.1 GHz	-135.0	-149.8	Band 0
2.1 to 3.6 GHz	-134.0	-148.8	Band 0
3.5 to 8.4 GHz	-126.2	-141.0	Band 1
8.3 to 13.6 GHz	-126.2	-141.0	Band 2
13.5 to 17.1 GHz	-125.2	-140.0	Band 3
17 to 20 GHz	-124.2	-139.0	Band 4
20 to 26.5 GHz	-117.7	-132.5	Band 4
26.4 to 30 GHz	-113.7	-128.5	Band 5
30 to 34 GHz	-111.7	-126.5	Band 5
33.9 to 37 GHz	-109.7	-124.5	Band 6
37 to 40 GHz	-99.7	-114.5	Band 6
40 to 44 GHz	-97.7	-112.5	Band 6
44 to 46 GHz	-96.7	-111.5	Band 6
46 to 50 GHz	-95.7	-110.5	Band 6
Linearity		$\pm (0.009 \text{ dB} + 0.005 \text{ dB}/10 \text{ dB step})^7$	
Relative measurement accuracy	Residual noise threshold ⁸ to maximum power	$\pm (0.015 \text{ dB} + 0.005 \text{ dB}/10 \text{ dB step})^{7,9,10}$ (nominal)	
	Minimum power to residual noise threshold	$\pm (\text{cumulative error}^{11} + 0.0012 \times (\text{input power} - \text{residual noise threshold power})^2)$	
Residual noise threshold power (dBm)	Residual noise threshold power = minimum power +30 dB		
Range 2 uncertainty ¹²	$\pm 0.031 \text{ dB}$		
Range 3 uncertainty ¹³	$\pm 0.031 \text{ dB}$		

- PXA Option N9030B-MPB is required to perform Tuned RF Level measurements above 3.6 GHz.
- These specifications are valid when the measuring receiver input is a CW tone and operating temperature is within the range of 20 to 30 °C.
- Absolute and relative accuracy specifications do not include mismatch uncertainty.
- With 30 kHz and 200 kHz IF bandwidth (IFBW), TRFL minimum power level will be degraded by a factor of $10\log(\text{IFBW}/75 \text{ Hz})$, relative to the specified 75 Hz minimum power level. This will result in a degradation of 26 dB for the 30 kHz IFBW and 34 dB for the 200 kHz IFBW.
- With 75 Hz IFBW setting selected, the measurement automatically switches the RBW to the 30 Hz setting for SNR values < 10 dB.
- With 10 Hz IFBW setting selected, the measurement automatically switches the RBW to the 1 Hz setting for SNR values < 10 dB.
- Step in this specification refers to the difference between relative measurements, such as might be experienced by stepping a stepped attenuator. Therefore, accuracy is computed by adding the uncertainty for each full or partial 10 dB step to the other uncertainty term. For example, if the two levels whose relative level is to be determined differ by 15 dB, consider that to be a difference of two 10-dB steps.
- The residual noise threshold power is the power level at which the signal-to-noise ratio (SNR) becomes the dominant contributor to the measurement uncertainty. See TRFL Specifications Nomenclature at the beginning of this section.
- Immediately following the system alignments, the measurement is made by manually setting frequency to that of the signal-under-test, Accuracy mode to High, and Measure Control to Single. Additionally, for the PXA with mmW frequency option, if the change of measured frequency crosses frequency bands, allow 10 minutes for thermal stability before taking the first measurement within the new band.
- This includes the linearity accuracy.
- In relative accuracy of TRFL measurements, the cumulative error is the error incurred when stepping from a higher power level to the Residual Noise Threshold Power level. The formula to calculate the cumulative error is $\pm (0.015 \text{ dB} + 0.005 \text{ dB}/10 \text{ dB step})$. For example, assume the higher level starting power is 0 dBm and the calculated Residual Noise Threshold Power is -99 dBm. The cumulative error would be $\pm (0.015 + \lceil 99/10 \rceil \times 0.005 \text{ dB})$, or $\pm 0.065 \text{ dB}$, where $\lceil x \rceil$ is a ceiling function that means the smallest integer is not less than x.
- Add this specification when the measuring receiver enters the Range 2 state. Range 2 is entered when the Range 1 signal-to-noise ratio (SNR) falls between 50 and 28 dB. The SNR value is tuning band dependent. A prompt of Range 2 in the PXA display will indicate that the measuring receiver is in Range 2.
- Add this specification in addition to Range 2 Uncertainty when the measuring receiver software enters the Range 3 state. Range 3 is entered when the Range 2 SNR falls between 50 and 28 dB. The SNR value is tuning band dependent. A prompt of Range 3 in the PXA display will indicate that the measuring receiver is in Range 3.

Key Specifications (continued)

1.12 Tuned RF level (continued)

Description	Specification	Supplemental Information
Absolute measurement accuracy	+20 dBm to maximum power	± (power meter range 1 uncertainty + 0.005 dB/10 dB step)
	Residual noise threshold power to +20 dBm	± (power meter range 2 - 4 uncertainty + 0.005 dB/10 dB step)
	Minimum power to residual noise threshold power	± (cumulative error ¹ + 0.0012 x (input power - residual noise threshold power) ²)
Residual noise threshold power (dBm)		Residual Noise Threshold Power = Minimum Power + 30 dB
Range 2 uncertainty ²	± 0.031 dB	
Range 3 uncertainty ³	± 0.031 dB	

1. In absolute accuracy of TRFL measurements, the cumulative error is the error incurred when stepping from a higher power level to the Residual Noise Threshold power level. See Figure 1 for a graphic. In order to calculate the cumulative error, you must determine the Residual Noise Threshold power and determine the Power Meter Range. The formula to calculate the cumulative error is: ± (Power Meter Range Uncertainty + 0.005 dB/10 dB step). For example: the power sensor is Option 504, starting power is 0 dBm and power will be stepped to -120 dBm. Therefore starting power falls in the Power Meter Range 2-4 and the uncertainty is ± 0.190 dB, as indicated in the table on the next page. The Residual Noise Threshold Power is -106 dBm at IFBW of 10 Hz. This is calculated per the Minimum Power specification in the table on the previous page. Assume no preamp is installed, and that the measurement frequency is 10 MHz to 3 GHz. The Residual Noise Threshold Power is -136 dBm + 30 dB = -106 dBm using the formula on this page. The cumulative error is then ± (0.190 dB + [106/10] x 0.005 dB), or ± 0.245 dB, where [x] is a ceiling function that means the smallest integer not less than x, which is 11 in this example.
2. Add this specification when the Measuring Receiver enters the Range 2 state. Range 2 is entered when the Range 1 signal-to-noise ratio (SNR) falls between 50 and 28 dB. The SNR value is tuning band dependent. A prompt of Range 2 in the PXA display will indicate that the Measuring Receiver is in Range 2.
3. Add this specification in addition to Range 2 Uncertainty when the Measuring Receiver enters the Range 3 state. Range 3 is entered when the Range 2 SNR falls between 50 and 28 dB. The SNR value is tuning band dependent. A prompt of Range 3 in the PXA display will indicate that the Measuring Receiver is in Range 3.

NOTE

As the displayed average noise level (DANL) of a spectrum/signal analyzer becomes very low, it can reveal residuals. These occur at discrete frequencies and arise from the various clocks and other components of the local oscillators. This is true for all modern spectrum/signal analyzers. The residuals specification for the PXA Series is -100 dBm. Please take this information into consideration when you measure the TRFL level below -100 dBm. A user may apply a 50-ohm terminator to the PXA's RF input connector and switch to the PXA's spectrum analysis mode to verify the PXA residuals.

Key Specifications (continued)

1.12 Tuned RF level (continued)

Description	Specification				Supplemental Information			
Power meter uncertainty (dB)								
Power meter range 1 (+20 to +30 dBm)					Typicals			
	Sensor module options				Sensor module options			
	504	518	526	550	504	518	526	550
100 kHz $\leq f_c \leq 10$ MHz	± 0.287	—	—	—	± 0.146	—	—	—
10 MHz $< f_c \leq 30$ MHz	± 0.287	± 0.287	$\pm 0.287^1$	—	± 0.146	± 0.146	$\pm 0.146^1$	—
30 MHz $< f_c \leq 2$ GHz	± 0.287	± 0.287	± 0.287	± 0.265	± 0.146	± 0.146	± 0.146	± 0.135
2 GHz $< f_c \leq 4.2$ GHz	± 0.302	± 0.302	± 0.302	± 0.279	± 0.154	± 0.154	± 0.154	± 0.142
4.2 GHz $< f_c \leq 18$ GHz	—	± 0.466	± 0.468	± 0.342	—	± 0.240	± 0.241	± 0.175
18 GHz $< f_c \leq 26.5$ GHz	—	—	± 0.386	± 0.332	—	—	± 0.198	± 0.170
26.5 GHz $< f_c \leq 50$ GHz	—	—	—	± 0.363	—	—	—	± 0.186
Power meter range 2 (0 to +20 dBm)					Typicals			
	Sensor module Options				Sensor module Options			
	504	518	526	550	504	518	526	550
0 to +20 dBm								
100 kHz $\leq f_c \leq 10$ MHz	± 0.222	—	—	—	± 0.113	—	—	—
10 MHz $< f_c \leq 30$ MHz	± 0.222	± 0.222	$\pm 0.222^1$	—	± 0.113	± 0.113	$\pm 0.113^1$	—
30 MHz $< f_c \leq 2$ GHz	± 0.222	± 0.222	± 0.222	± 0.191	± 0.113	± 0.113	± 0.113	± 0.097
2 GHz $< f_c \leq 4.2$ GHz	± 0.242	± 0.242	± 0.242	± 0.211	± 0.123	± 0.123	± 0.123	± 0.107
4.2 GHz $< f_c \leq 18$ GHz	—	± 0.432	± 0.433	± 0.291	—	± 0.222	± 0.232	± 0.148
18 GHz $< f_c \leq 26.5$ GHz	—	—	± 0.342	± 0.279	—	—	± 0.175	± 0.142
26.5 GHz $< f_c \leq 50$ GHz	—	—	—	± 0.316	—	—	—	± 0.161
Power meter range 3 (-5 to 0 dBm)					Typicals			
	Sensor module options				Sensor module options			
	504	518	526	550	504	518	526	550
100 kHz $\leq f_c \leq 10$ MHz	± 0.220	—	—	—	± 0.112	—	—	—
10 MHz $< f_c \leq 30$ MHz	± 0.220	± 0.219	$\pm 0.220^1$	—	± 0.112	± 0.111	$\pm 0.112^1$	—
30 MHz $< f_c \leq 2$ GHz	± 0.220	± 0.219	± 0.220	± 0.189	± 0.112	± 0.111	± 0.112	± 0.096
2 GHz $< f_c \leq 4.2$ GHz	± 0.240	± 0.240	± 0.240	± 0.209	± 0.122	± 0.122	± 0.122	± 0.106
4.2 GHz $< f_c \leq 18$ GHz	—	± 0.430	± 0.432	± 0.289	—	± 0.221	± 0.222	± 0.148
18 GHz $< f_c \leq 26.5$ GHz	—	—	± 0.341	± 0.277	—	—	± 0.174	± 0.141
26.5 GHz $< f_c \leq 50$ GHz	—	—	—	± 0.315	—	—	—	± 0.161
Power meter range 4 (-10 to -5 dBm)					Typicals			
	Sensor module options				Sensor module options			
	504	518	526	550	504	518	526	550
100 kHz $\leq f_c \leq 10$ MHz	± 0.229	—	—	—	± 0.117	—	—	—
10 MHz $< f_c \leq 30$ MHz	± 0.229	± 0.229	$\pm 0.229^1$	—	± 0.117	± 0.117	$\pm 0.117^1$	—
30 MHz $< f_c \leq 2$ GHz	± 0.229	± 0.229	± 0.229	± 0.200	± 0.117	± 0.117	± 0.117	± 0.102
2 GHz $< f_c \leq 4.2$ GHz	± 0.249	± 0.249	± 0.249	± 0.219	± 0.127	± 0.127	± 0.127	± 0.111
4.2 GHz $< f_c \leq 18$ GHz	—	± 0.435	± 0.437	± 0.296	—	± 0.224	± 0.225	± 0.151
18 GHz $< f_c \leq 26.5$ GHz	—	—	± 0.347	± 0.285	—	—	± 0.178	± 0.145
26.5 GHz $< f_c \leq 50$ GHz	—	—	—	± 0.321	—	—	—	± 0.164

1. For U5532C USB sensor modules only.

Key Specifications (continued)

1.12 Tuned RF level (continued)

Description	Specification	Supplemental Information
Operating frequency range		
Option N9030B-503/508/513/526/544/550	100 kHz to 3.6 GHz	
N9030B-508/513/526/544/550	3.6 to 8.4 GHz	Requires Option N9030B-MPB
N9030B-513/526/544/550	8.4 to 13.6 GHz	Requires Option N9030B-MPB
Option N9030B-526/544/550	13.6 to 26.5 GHz	Requires Option N9030B-MPB
Option N9030B-544/550	26.5 to 44 GHz	Requires Option N9030B-MPB
N9030B	44 to 50 GHz	Requires Option N9030B-MPB
Displayed units	Absolute	Watts, dBm, or Volts
	Relative	Percent or dB
Displayed resolution	6 digits in Watts or 5 digits in Volts mode	
	0.001 dB in dBm or dB (relative) mode	
Input SWR	See "RF Power" Section	

N5531X Ordering Information

For the N5531X with the primary configuration: order an N9030B PXA and a U5532C USB sensor module;

For the N5531X with the alternative configuration: order an N9030B PXA, a power meter, and an N5532B sensor module.

N9030B PXA signal analyzer, multi-touch

Select one of the following frequency options

- N9030B-503: 2 Hz to 3.6 GHz
- N9030B-508: 2 Hz to 8.4 GHz
- N9030B-513: 2 Hz to 13.6 GHz
- N9030B-526: 2 Hz to 26.5 GHz
- N9030B-544: 2 Hz to 44 GHz
- N9030B-550: 2 Hz to 50 GHz

Other PXA options

N9030B-MPB

Microwave preselector bypass (required for TRFL measurements above 3.6 GHz)

N9030B-P03/P08/P13/P26/P44/P50

Preamplifier (required for the best TRFL specifications up to the maximum frequency of the PXA frequency option covers)

The N5531X ordering system automatically selects a preamplifier option to cover up to the maximum frequency defined by the PXA frequency option

- N9030B-P03 Preamplifier, 3.6 GHz
- N9030B-P08 Preamplifier, 8.4 GHz
- N9030B-P13 Preamplifier, 13.6 GHz
- N9030B-P26 Preamplifier, 26.5 GHz
- N9030B-P44 Preamplifier, 44 GHz
- N9030B-P50 Preamplifier, 50 GHz

N9030B-107

Audio input and digitizer (required for audio analysis, only operational with N9091EM0E measuring receiver application or with N9092EM0E avionics measurement application)

N9030B-033

Measuring receiver connector accessory kit, 26.5 GHz (Optional) provides a set of metrology-grade coaxial connector adapters including quantity 2 of each: type-N (f) to 3.5 mm (f), APC-7 to APC-3.5 (f), 3.5 mm (f) to 3.5 mm (f), 3.5 mm (m) to 3.5 mm (f); and a 3.5 mm (m-f) RF cable assembly.

N9030B-034

Measuring receiver connector accessory kit, 50 GHz (Optional) provides a set of metrology-grade coaxial connector adapters including quantity 2 of each: type-N (f) to 2.4 mm (f), APC-7 to 2.4 mm (f), 2.4 mm (f) to 3.5 mm (f), 2.4 mm (f) to 3.5 mm (f), 2.4 mm (f) to 3.5 mm (m); and a 2.4 mm (m-f) 50 GHz cable assembly.

X-Series measurement applications

N9091EM0E

X-Series measuring receiver application (required for measuring receiver)

PXA option upgrades¹

N9030BU-MPB

Microwave preselector bypass (required for TRFL measurements above 3.6 GHz, if the PXA (with any frequency option) has Opt LNP installed), or

N9030BU-HL1

Microwave preselector bypass (required for TRFL measurements above 3.6 GHz, if the PXA (with option 508/513/526) does not have Opt LNP installed), or

N9030BU-HL2

Microwave preselector bypass (required for TRFL measurements above 3.6 GHz, if the PXA (with option 544/550) does not have Opt LNP installed)

N9030BU-P03/P08/P13/P26/P44/P50

Preamplifier (required for the best TRFL specifications up to the maximum frequency of the PXA base instrument)

N9030BU-107

Audio input and digitizer (required for audio analysis, only operational with N9091EM0E, or with N9092EM0E)

U5532C USB sensor module (for the primary configuration)

(Select frequency option)

U5532C-504

100 kHz to 4.2 GHz USB sensor module, type-N (m) input connector

U5532C-518

10 MHz to 18 GHz USB sensor module, type-N (m) input connector

U5532C-526

10 MHz to 26.5 GHz USB sensor module, APC-3.5 (m) input connector

U5532C-550

30 MHz to 50 GHz USB sensor module, 2.4 mm (m) input connector

Select from U5532C options (optional)

Power meter (for the alternative configuration)

(Select one model)

N1913A

EPM Series single channel power meter

N1914A

EPM Series dual channel power meter

N1911A

P-Series single channel power meter

N1912A

P-Series dual channel power meter

Select from power meter options (optional)

1. For the existing N9030B PXA only. Upgrades for certain PXA options may not be available for earlier instruments. For detailed information regarding availability and compatibility of options, please visit http://www.keysight.com/find/pxa_upgrades

N5532B sensor module (for the alternative configuration)

(Select frequency option)

N5532B-504

100 kHz to 4.2 GHz, type-N (m) input connector

N5532B-518

10 MHz to 18 GHz, type-N (m) input connector

N5532B-526

30 MHz to 26.5 GHz, APC-3.5 (m) input connector

N5532B-550

30 MHz to 50 GHz, 2.4 mm (m) input connector

N5532B-019

Adaptor to N1911A/12A power meter (required when the N1911A/12A P-Series power meter is used), can also be ordered standalone

Select from N5532B options (optional)

Related Literature

Publication title	Publication type	Publication number
N5531X in general		
N5531X X-Series measuring receiver configuration guide	Configuration Guide	5992-2675EN
PXA in general		
PXA X-Series Signal Analyzer, Multi-touch N9030B	Configuration Guide	5992-1318EN
Power meter in general		
N1913A/N1914A EPM Power Meters	Data Sheet	5990-4019EN
N1911A/N1912A P-Series Power Meters	Data Sheet	5989-2471EN
Power measurement fundamentals		
Fundamentals of RF and Microwave Power Measurements, Introduction to Power, History, Definition, International Standards, and Traceability	Application Note 1449-1	5988-9213EN
Fundamentals of RF and Microwave Power Measurements, Power Sensors and Instrumentation	Application Note 1449-2	5988-9214EN
Fundamentals of RF and Microwave Power Measurements, Power Measurement Uncertainty per International Guides	Application Note 1449-3	5988-9215EN
Fundamentals of RF and Microwave Power Measurements, An Overview of Agilent Instrumentation for RF/Microwave Power Measurement	Application Note 1449-4	5988-9216EN

Learn more at: www.keysight.com

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

